




ID1	ID2	Type	No. Spec	Est. Comp			
RBS146	RBS0146	* (S?)	20	68%			
[dir/date]	[medRA]	[medDEC]	[PA]	[dRA]	[dDEC]	[SCAN]	[N]
2012_01_19_20	01:02:50.40	-72:01:56.59	0.0	-15.7	-15.4	E2W-N2S	6
2012_01_20_21	01:02:48.10	-72:01:56.21	0.0	-17.6	-17.3	E2W-N2S	7
2012_01_21_22	01:02:45.50	-72:02:15.10	0.0	-18.5	-17.2	E2W-N2S	7

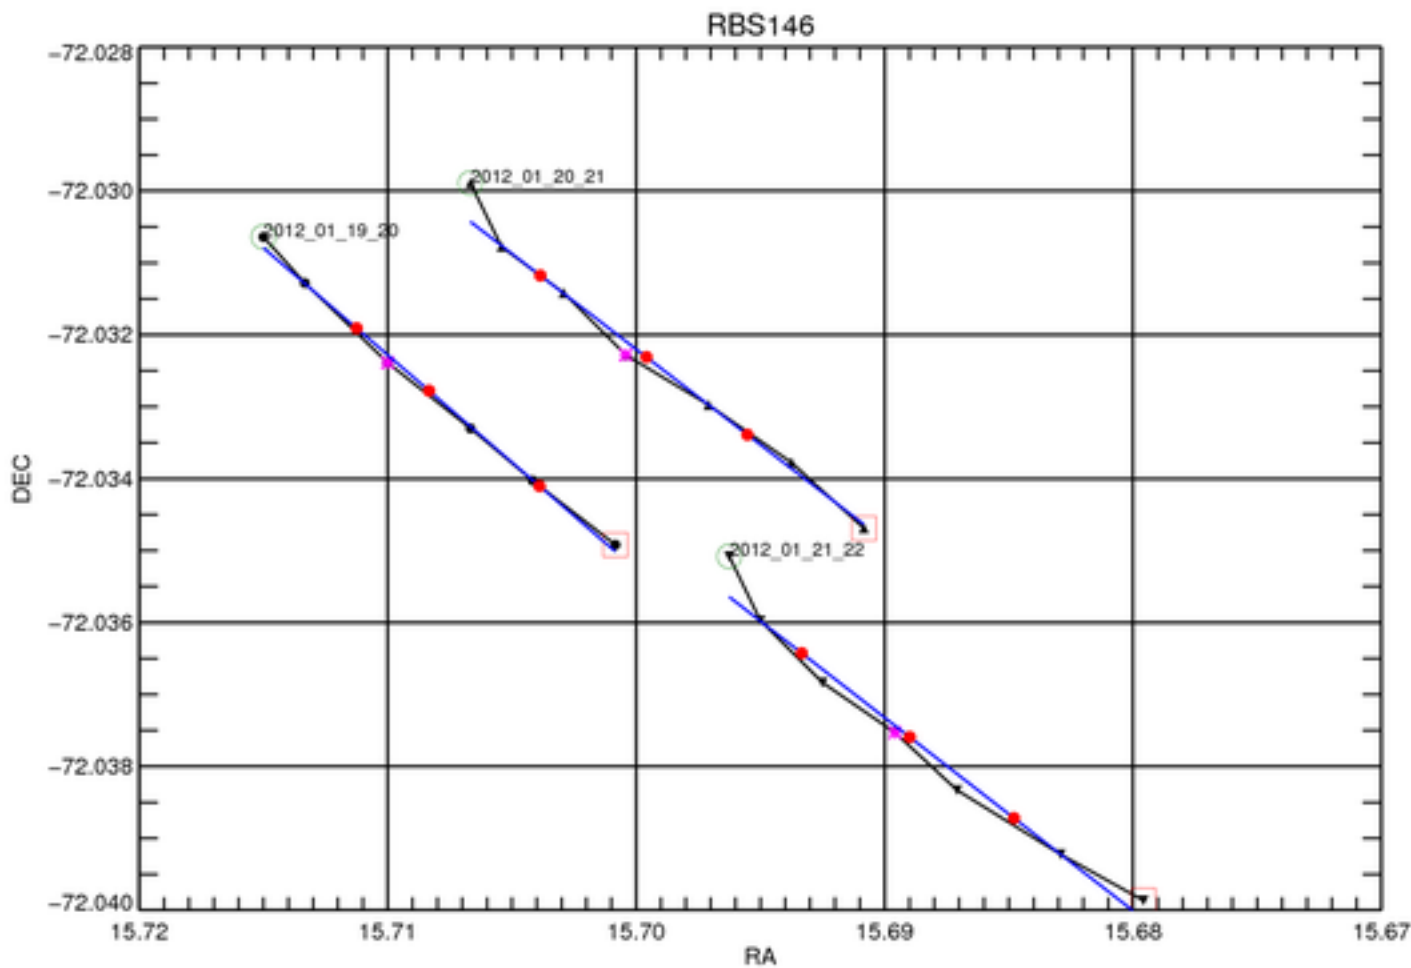

RBS146 VIS 2012 01 19 20

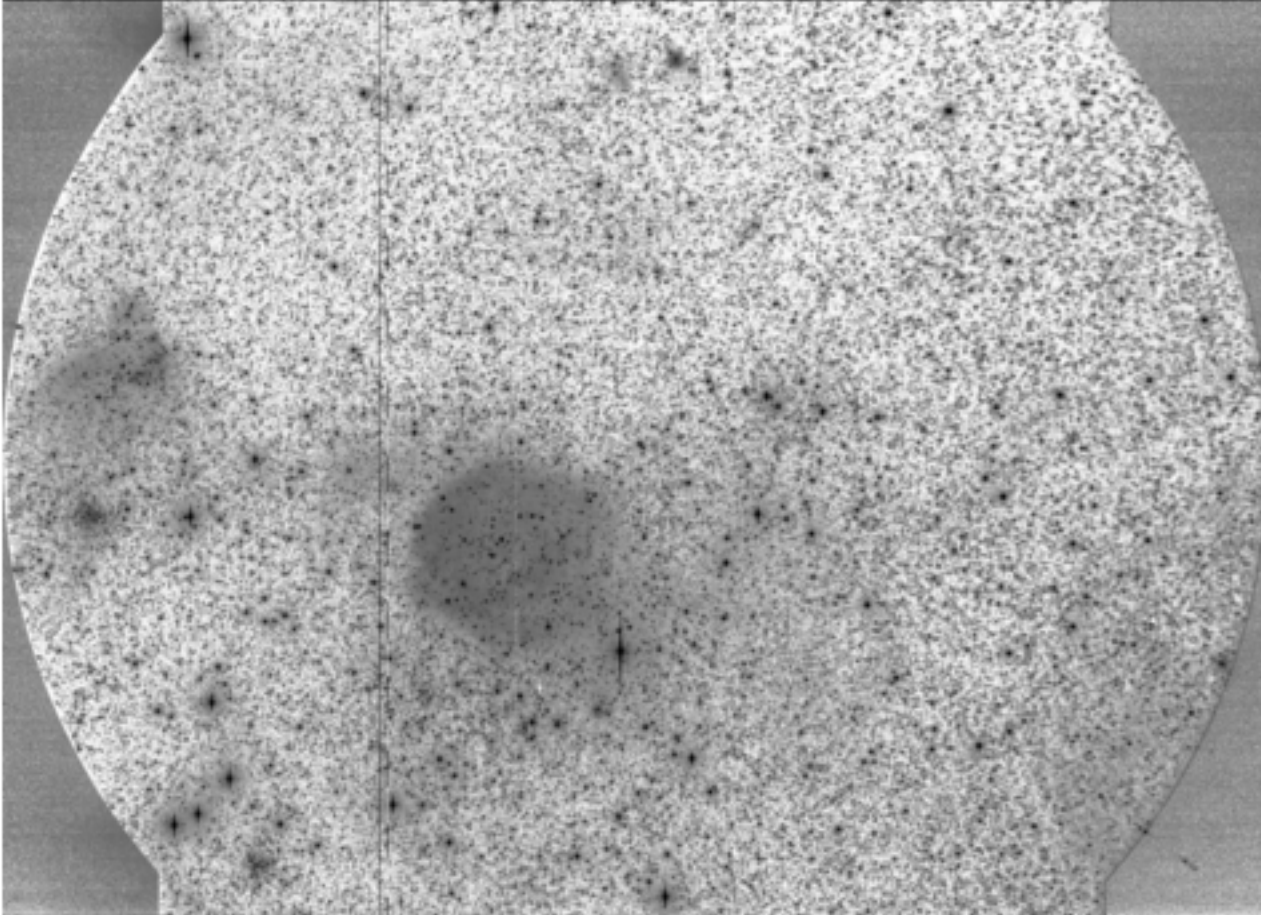

RBS146_VIS_2012_01_20_21

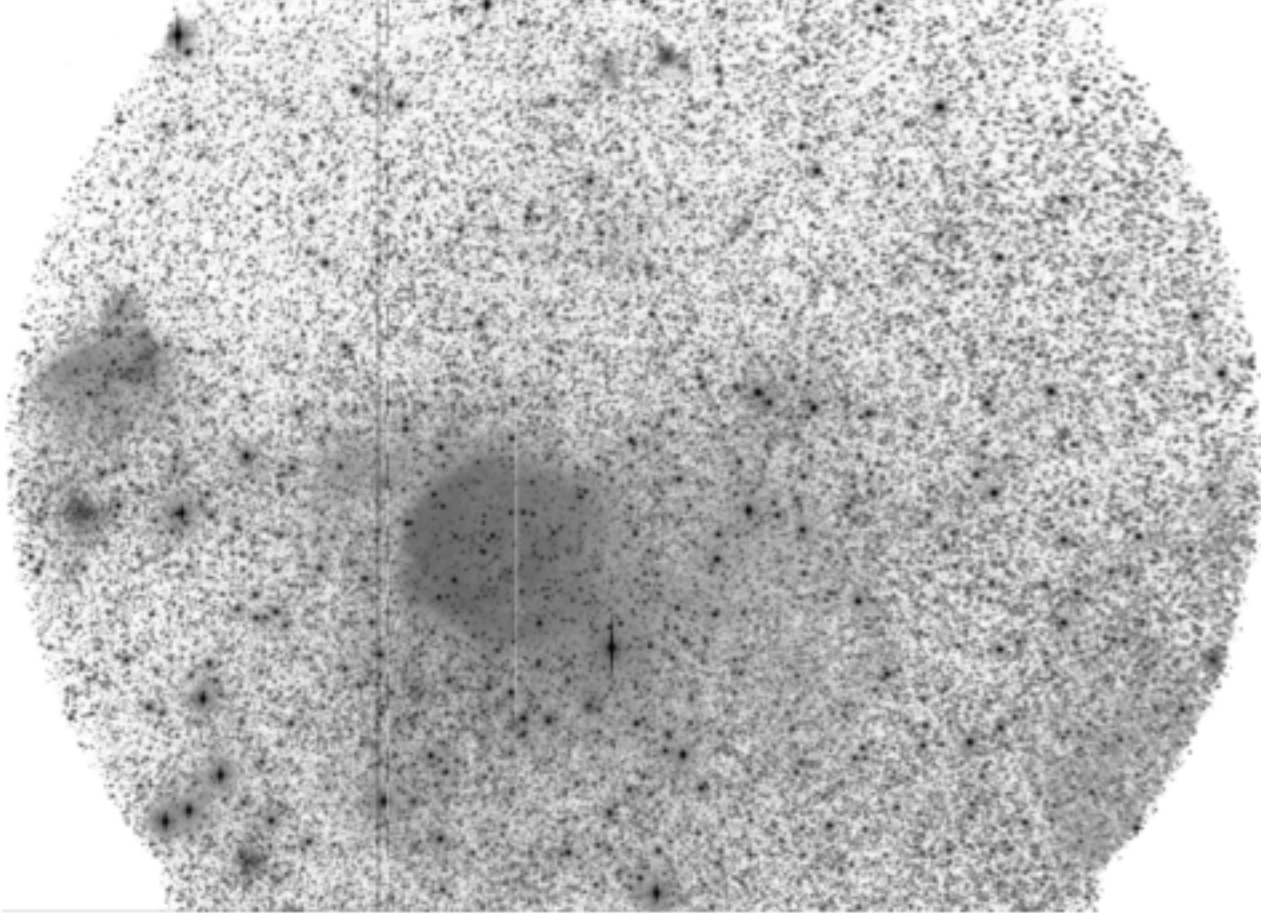

RBS146_VIS_2012_01_21_22

